


Keysight Technologies

Low Frequency RFID Tag Characterization

Using the N9322C Basic Spectrum Analyzer (BSA)

Application Note

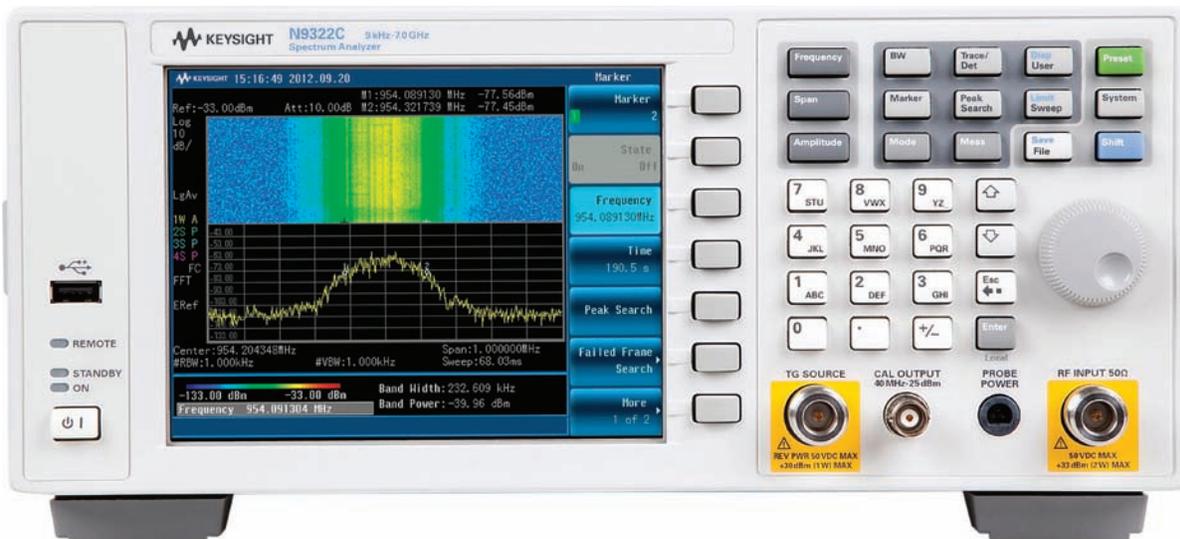

About RFID Tags

Radio frequency ID (RFID) systems rely on RFID tags, which are small transponders (a combined radio receiver and transmitter) that transmit identity information over a short distance when asked. Generally, an RFID tag contains two parts. One is an integrated circuit for storing and processing information, and modulating and de-modulating an RF signal. Another part is an antenna for receiving and transmitting signals to the reader (see Figure 1).

The resonance frequency of the RFID tag is one of the key factors that impact the effective communication distance between the reader and RFID tags. When RFID tags are packaged, a non-contact coupling method can be used to measure their resonance frequencies, which corresponds to the negative peak of its return loss characteristic curve.

Abstract

The resonance frequency of a radio frequency identification (RFID) tag is a key factor that determines the effective radio communication distance between the tag and the reader. Measuring the resonance frequency of an RFID tag is easy using the Keysight Technologies, Inc. N9322C basic spectrum analyzer (BSA).

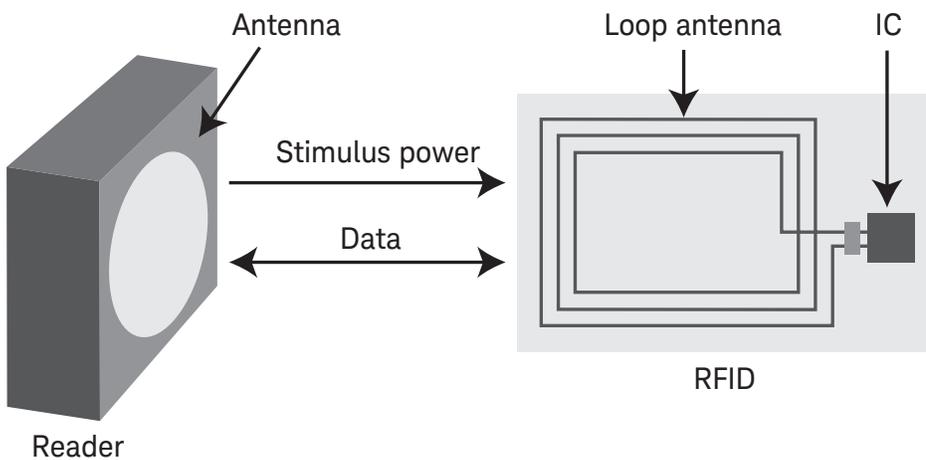


Figure 1. An overview of an RFID system

Measuring a 13.56 MHz Passive RFID Tag with the N9322C Basic Spectrum Analyzer (BSA)

The N9322C is a multi-use RF analyzer that spans to spectrum analysis, transmission measurement, and reflection measurement. By simply adding the tracking generator (Option TG7) and the reflection measurement application (Option RM7), the N9322C BSA is capable of measuring the return loss of RFID tags:

- The Option TG7 tracking generator contains a built-in VSWR bridge, which makes the reflection measurement more convenient to perform using the N9322C BSA versus using other analyzers that require an external bridge.
- In addition, the N9322C's reflection measurement mode uses a high precision open-short-load (OSL) calibration procedure, which greatly reduces system errors.

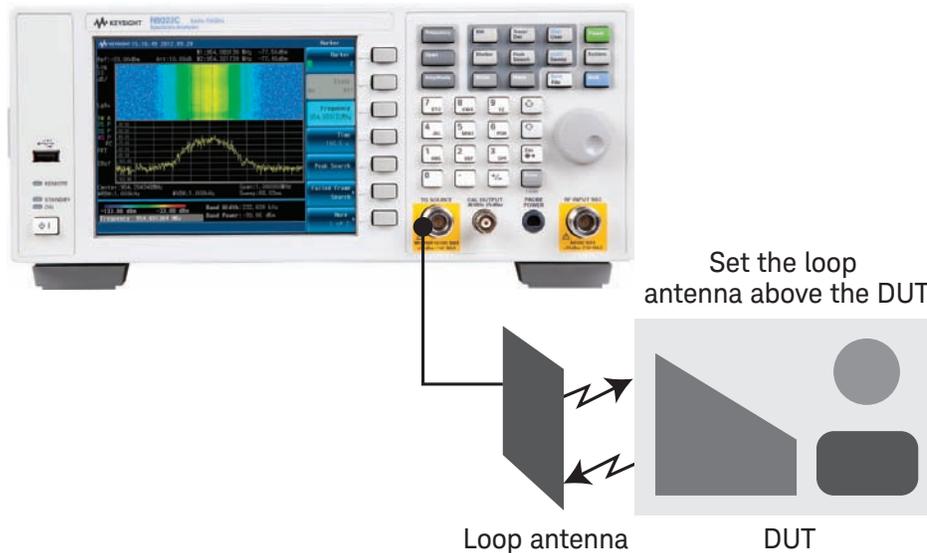


Figure 2. Simple test setup for reflection measurements

Demonstration: Measuring an RFID Tag with the N9322C BSA

- In this demonstration, we utilized a 13.56 MHz RFID tag, which follows the ISO/IEC 14443 type A standard.
- In the following demonstration procedure, text in [] refers to a hardkey and { } refers to a softkey on the N9322C spectrum analyzer.
- Instrument and accessories used in this demonstration include:
 - N9322C basic spectrum analyzer (BSA), with Options TG7 and RM7 enabled
 - N9311X-201 precision mechanical open-short-load (OSL) calibrator
 - Near field probe (used for radiating RF power from the tracking generator to activate the RFID tag)
 - A sample RFID tag (13.56 MHz)
 - E5071C ENA network analyzer (used to compare the measurement result to that obtained using the N9322C)

Step 1. Set up the measurement parameters

- Press [Mode] > {Reflection measurement}
- Press [Frequency] > {Start Freq} > [12] > {MHz} to set the start frequency to 12 MHz
- Press [Frequency] > {Stop Freq} > [15] > {MHz} to set the stop frequency to 15 MHz
- Toggle the {Cal. Type} to {Selected} in order to achieve the highest calibration accuracy within the frequency range of interest

Step 2. Calibrate the N9322C BSA

- Press {Calibrate} and follow the instructions on the BSA to calibrate with the OSL calibrator (product number: N9311X-201)
- When finished, a “Calibrated” mark displays in the left upper corner of the screen
- Press [Amplitude] > {Scale/DIV} > [2] > {dB} to display the amplitude scale for easier observation




Connect the **OPEN** and **TG SOURCE** as shown.
Once connected, press **[ENTER]** to continue, or **[ESC]** to abort.

Figure 3. Performing OSL calibration on the N9322C BSA

Step 3. Start measurement using a near field probe

- Connect the near field probe to the TG Output port of the N9322C BSA, and place the probe about 1 cm (0.4 in) above the sample RFID tag (see Figure 4)
- Use the Marker on the N9322C BSA to read the negative peak of the trace. You can also verify the measurement result using an E5071C ENA (see Figures 5 and 6)

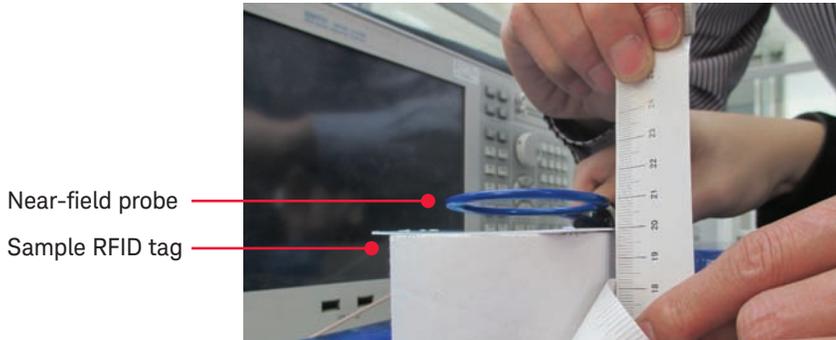

Connect the **OPEN** and **TG SOURCE** as shown. Once connected, press **[ENTER]** to continue, or **[ESC]** to abort.

Figure 4. Use a close-field probe as the power radiator and collector



Figure 5. Return loss result measured with the N9322C BSA

myKeysight

myKeysight

www.keysight.com/find/mykeysight

A personalized view into the information most relevant to you.

Three-Year Warranty

www.keysight.com/find/ThreeYearWarranty

Keysight's commitment to superior product quality and lower total cost of ownership. The only test and measurement company with three-year warranty standard on all instruments, worldwide.



Keysight Assurance Plans

www.keysight.com/find/AssurancePlans

Up to five years of protection and no budgetary surprises to ensure your instruments are operating to specification so you can rely on accurate measurements.



www.keysight.com/go/quality

Keysight Technologies, Inc.
DEKRA Certified ISO 9001:2008
Quality Management System



Keysight Channel Partners

www.keysight.com/find/channelpartners

Get the best of both worlds: Keysight's measurement expertise and product breadth, combined with channel partner convenience.

www.keysight.com/find/n9322c

For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: www.keysight.com/find/contactus

Americas

Canada	(877) 894 4414
Brazil	55 11 3351 7010
Mexico	001 800 254 2440
United States	(800) 829 4444

Asia Pacific

Australia	1 800 629 485
China	800 810 0189
Hong Kong	800 938 693
India	1 800 112 929
Japan	0120 (421) 345
Korea	080 769 0800
Malaysia	1 800 888 848
Singapore	1 800 375 8100
Taiwan	0800 047 866
Other AP Countries	(65) 6375 8100

Europe & Middle East

Austria	0800 001122
Belgium	0800 58580
Finland	0800 523252
France	0805 980333
Germany	0800 6270999
Ireland	1800 832700
Israel	1 809 343051
Italy	800 599100
Luxembourg	+32 800 58580
Netherlands	0800 0233200
Russia	8800 5009286
Spain	800 000154
Sweden	0200 882255
Switzerland	0800 805353
	Opt. 1 (DE)
	Opt. 2 (FR)
	Opt. 3 (IT)
United Kingdom	0800 0260637

For other unlisted countries:
www.keysight.com/find/contactus
(BP-09-23-14)